

Test Group Summary Report

C01A Major Ions in Water

March 2020 PT Round

Issued: June 16, 2020

Table of Contents

1.0	The Proficiency Testing Report	1
2.0	Definitions	1
3.0	Scoring System	1
3.1	Homogeneity and Stability Assessment	2
3.2	The z score	2
3.2	Composite (PT) Score	2
3.3	Identifying Bias	2
3.4	Deviations from Evaluation Procedure	3
4.0	Study Specific Data Summary	3
4.1	Overall Data Distribution	3
4.2	z-Score Plots	3
4.3	Statistical Summary by Method	3
5.0	Summary by Analyte	4

1.0 The Proficiency Testing Report

The Proficiency Testing Report consists of two parts.

- *PTC Proficiency Testing Report:* This report contains participant-specific evaluations and other confidential information. This report is emailed to participants at the end of the study.
- *Test Group Summary Report:* A Test Group Summary Report is created for each test group at the end of the study. These reports contain more detailed information on the study than are found in the participant-specific PTC Proficiency Testing Report. These reports do not contain any confidential information and are made available on the PTC web site.

2.0 Definitions

The participant-specific PTC Proficiency Testing Report contains some terms that new participants may not be familiar with.

<i>Code:</i>	The registration code that is unique to each analyte that a participant is registered for.
<i>App:</i>	If a participant is accredited by CALA, this three digit number is the appendix number that the accredited method is assigned to.
<i>N:</i>	The number of participants results that were used to calculate the summary statistics. This excludes qualified data (e.g., <) and any results that were flagged as outliers.
<i>Assigned:</i>	The Assigned Value is the robust mean of the reported results, outliers excluded. This is often referred to as the “target” value.
<i>±u:</i>	The uncertainty of the assigned value.
<i>Reported:</i>	The result reported by the participant.
<i>s:</i>	The Standard Deviation of Proficiency Assessment. This value is used to determine the acceptance limits for the PT evaluation.
<i>z-Score:</i>	A value assigned to each reported result that is a measure of how much it deviates from the Assigned Value.
<i>Score:</i>	The composite score of the four results reported for each analyte. It is normalized to a score out of 100.
<i>Bias:</i>	A flag assigned if bias is detected using the re-scaled z-score procedure.

3.0 Scoring System

Participant performance is evaluated for each proficiency testing sample by a quantitative method that is consistent with ISO/IEC 17043:2010 *Conformity assessment – General requirements for proficiency testing*, the *International Harmonized Protocol for Proficiency Testing of (Chemical) Analytical Laboratories* (2006), and ISO 13528:2015 *Statistical methods for use in proficiency testing by interlaboratory comparisons*.

The following is a brief description of the evaluation procedure used by PTC. The detailed evaluation procedure is described in PROC09 - *Procedures*, which is available on the PTC website www.PTCanada.org).

3.1 HOMOGENEITY AND STABILITY ASSESSMENT

Homogeneity and stability are assessed using participant data. Regression analysis is performed on reported result against order of sample production (Homogeneity) and reported result against date of analysis (Stability). If the slope is significantly different than zero for either then the Standard Deviation of Proficiency Assessment (s) is increased until the impact is minimized.

3.2 THE Z SCORE

A "z-score" is calculated for each reported result as follows:

$$z = \frac{(x - \bar{X})}{s}$$

where: x = participant's result;
 \bar{X} = the Assigned Value for the sample;
 s = the Standard Deviation for Proficiency Assessment.

The assigned value \bar{X} is generally estimated from the inter-laboratory Robust mean after outliers due to obvious gross errors (e.g., reported in wrong units) have been removed.

The Standard Deviation for Proficiency Assessment, s , is determined as follows:

- The inter-laboratory Robust standard deviation (stdev) is calculated using reported results, obvious outliers removed;
- The expected inter-laboratory standard deviation ($s!$) is estimated from regression equations derived from previous studies (see PROC11- *PT Regression Equations* for details);
- If $s!$ is higher than stdev then $s!$ is used in the z score equation;
- If $s!$ is lower than stdev then stdev is used in the z score equation;
- When a laboratory reports its detection limit, s will be estimated using a pooled variance procedure that uses both the inter-laboratory data and the reported detection limit.

3.2 COMPOSITE (PT) SCORE

Since each PT study involves four or two separate samples of distinct concentrations for each test, it is necessary to calculate a composite PT score for each test to determine overall performance. The composite score is calculated by first averaging the absolute z-scores for the four results and then calculating a final score as $100 + (-15 \times \text{avg } |z|)$.

Acceptable PT Scores equal or exceed 70.

3.3 IDENTIFYING BIAS

The proficiency testing report provides flags for bias. These are determined using the re-scaled z-score procedure.

$$RSZ = \frac{\sum z}{\sqrt{N}}$$

where z = the z -score
 N = the number of samples

Flags are assigned for each test group/parameter combination as follows:

$RSZ \geq -2$ and ≤ 2	no flag assigned
$RSZ > 2$	H (High)
$RSZ > 3$	VH (Very High)
$RSZ < -2$	L (LOW)
$RSZ < -3$	VL (Very Low)

3.4 DEVIATIONS FROM EVALUATION PROCEDURE

Other than changes to the Standard Deviation of Proficiency Assessment due to homogeneity or stability flags, any deviation from the published evaluation procedure is described on the cover page(s) of the final PT report.

4.0 Study Specific Data Summary

The following pages provide more detailed information about the study indicated in the cover page of this report than is found in the participant-specific PTC Proficiency Testing Report. The graphical representations and the statistical summaries by method are based upon the data after outliers have been removed.

4.1 OVERALL DATA DISTRIBUTION

Kernel density plots are generated for each data set. These plots are a statistical way to represent the overall data distribution and are used to visualize deviations from normality and bi-modality.

4.2 z-SCORE PLOTS

The z -scores for each sample are ranked in increasing order and plotted. When the data is normally distributed, the plot should show a slight sigmoidal curve, with an equal number of points above zero as below.


4.3 STATISTICAL SUMMARY BY METHOD

Statistical summaries are provided for the four most commonly reported methods. The statistics included in these tables for mean and standard deviation are the mathematical values, not the robust values. As such, there will be slight differences between these and those displayed in the participant specific PTC Proficiency Testing Report.


In addition to this, z -Score plots are provided for the four most common methods. As these plots use the Assigned Value and Standard Deviation for Proficiency Assessment estimated using all of the data, any method that does not have approximately the same number of positive and negative z -scores is an indication that the method may be biased relative to other methods.

Alkalinity (pH 4.5)

Kernel Density Plots

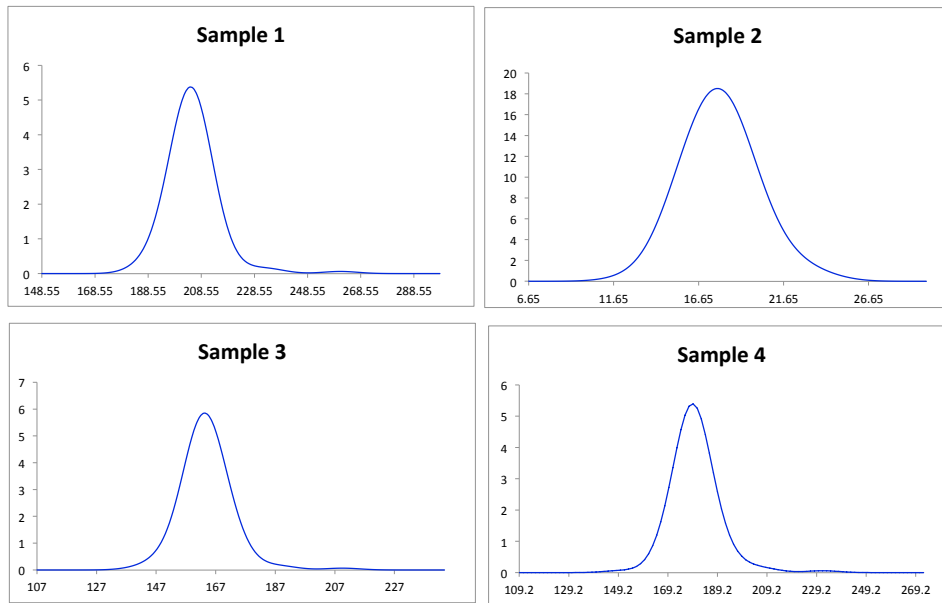

z-Score Plots

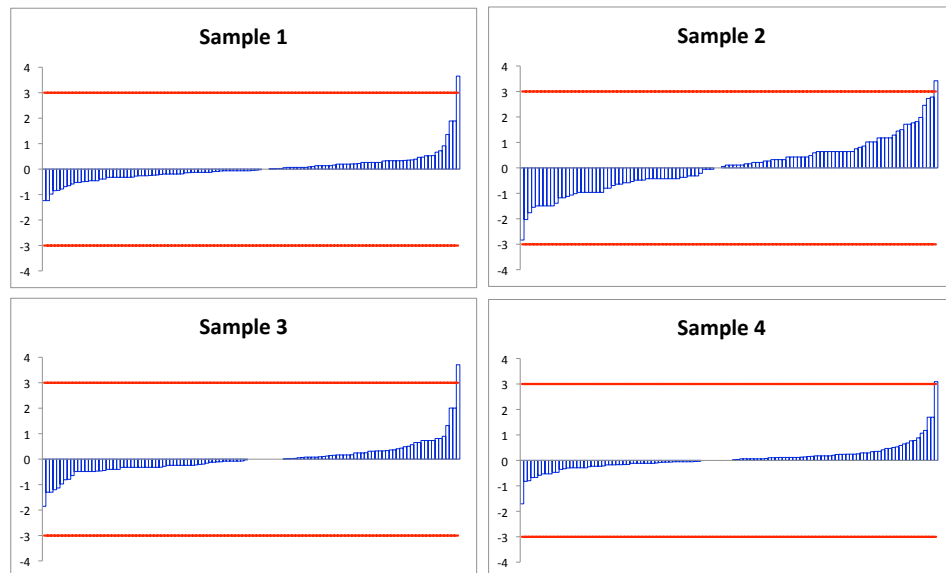

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	TITR	TITR-A	CLR-A	COLOR
Median	205	205	203	204	207
Stdev	15.3	10.2	6.49	6.05	6.61
Number	118	63	42	7	5
z > 3	1	1	0	0	0
z 2 - 3	0	0	0	0	0


Sample 2					
Method	All*	TITR	TITR-A	CLR-A	COLOR
Median	17.8	18	17.7	18.1	18.6
Stdev	1.87	2.01	2	1.89	1.66
Number	110	58	41	6	5
z > 3	1	0	1	0	0
z 2 - 3	5	4	1	0	0

Sample 3					
Method	All*	TITR	TITR-A	CLR-A	COLOR
Median	164	164	163	163	164
Stdev	12.3	9.54	5.3	5.63	5.73
Number	118	63	42	7	5
z > 3	1	1	0	0	0
z 2 - 3	2	2	0	0	0

Sample 4					
Method	All*	TITR	TITR-A	CLR-A	COLOR
Median	179	180	178	182	182
Stdev	17	10.3	6.11	6.82	4.56
Number	118	63	42	7	5
z > 3	1	1	0	0	0
z 2 - 3	0	0	0	0	0





* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4




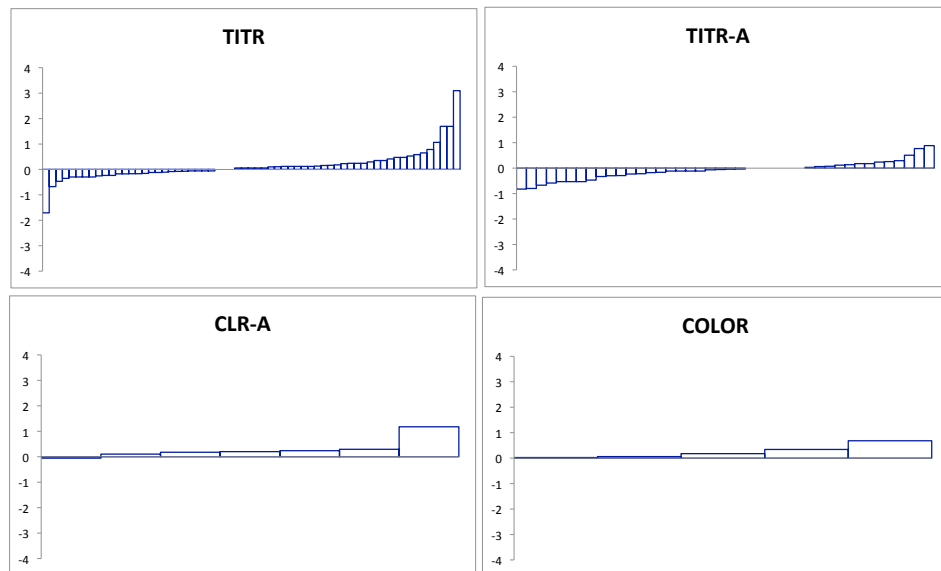


Calcium

Kernel Density Plots

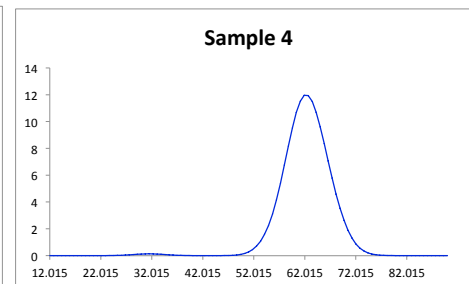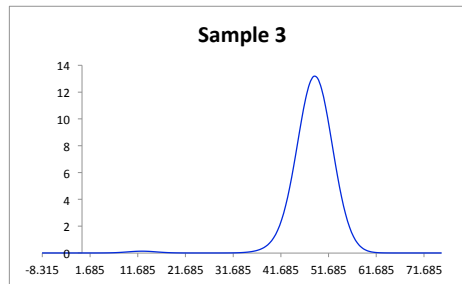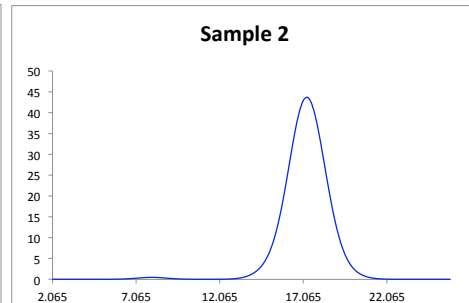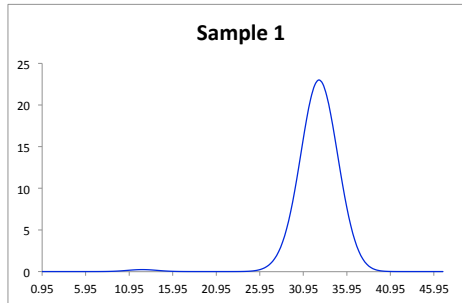

z-Score Plots

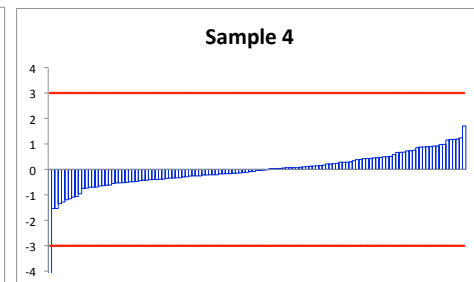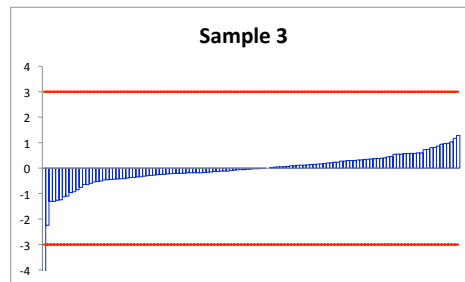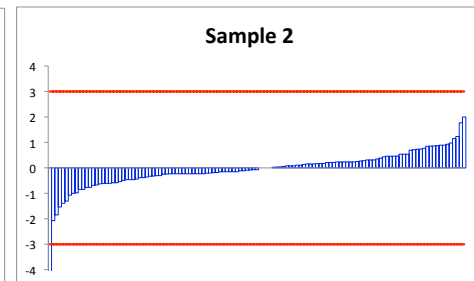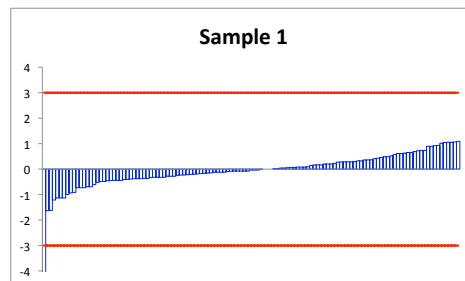

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	32.8	32.8	32.6	32.7	32.6
Stdev	2.46	1.36	1.44	1.06	11.9
Number	125	66	46	6	3
z > 3	1	0	0	0	1
z 2 - 3	0	0	0	0	0


Sample 2					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	17.3	17.3	17.2	17.3	16.5
Stdev	1.3	0.767	0.891	0.835	5.49
Number	125	66	46	6	3
z > 3	1	0	0	0	1
z 2 - 3	1	0	1	0	0

Sample 3					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	48.8	48.9	48.2	48.4	47.6
Stdev	4.36	2.13	2.79	2.24	20.7
Number	125	66	46	6	3
z > 3	1	0	0	0	1
z 2 - 3	1	0	1	0	0

Sample 4					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	62.5	62.7	61.7	62.8	61.7
Stdev	4.68	2.62	3.33	2.21	18.2
Number	125	66	46	6	3
z > 3	1	0	0	0	1
z 2 - 3	0	0	0	0	0


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

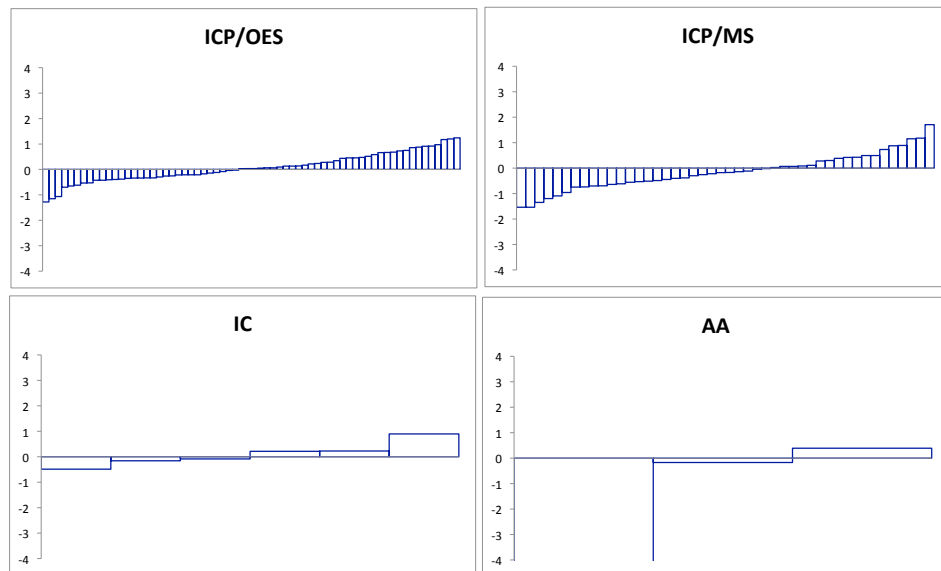


Chloride

Kernel Density Plots

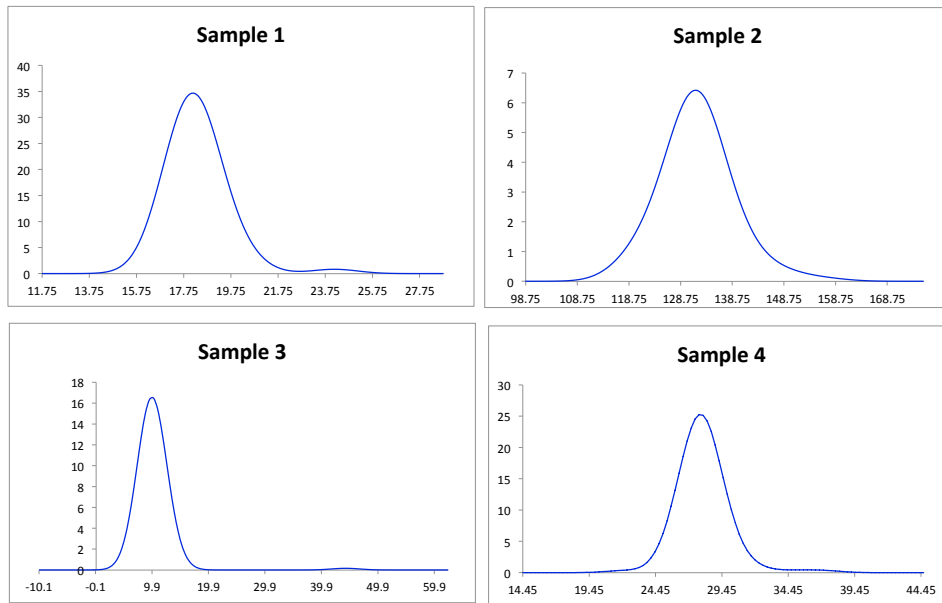

z-Score Plots

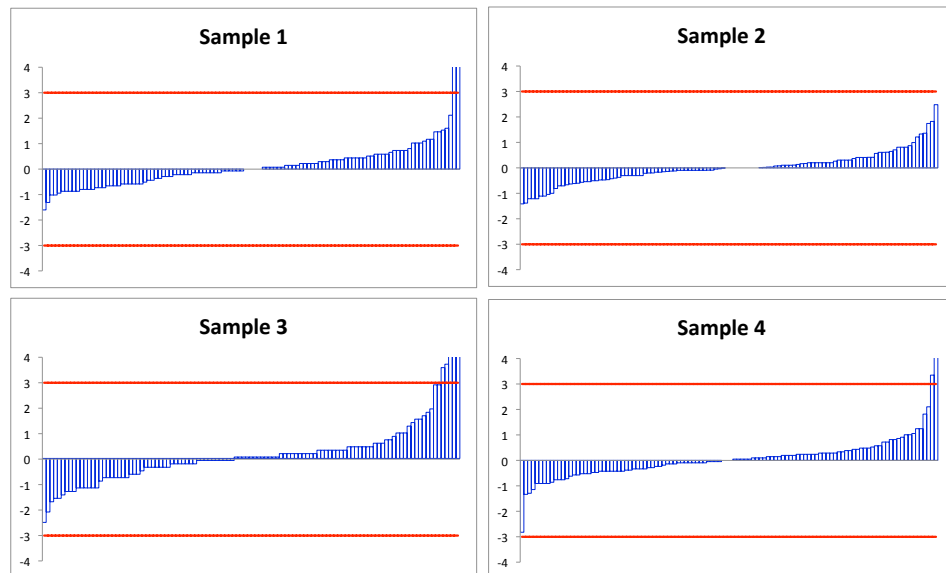

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	IC	TITR	COLOR	CLR-A
Median	18.2	18.1	19.2	18.7	17.6
Stdev	1.37	0.809	2.15	1.7	0.933
Number	112	75	12	11	10
z > 3	2	0	1	1	0
z 2 - 3	1	0	1	0	0


Sample 2					
Method	All*	IC	TITR	COLOR	CLR-A
Median	132	132	132	132	130
Stdev	9.88	5.86	7.94	6	3.55
Number	112	75	12	11	10
z > 3	0	0	0	0	0
z 2 - 3	1	1	0	0	0

Sample 3					
Method	All*	IC	TITR	COLOR	CLR-A
Median	9.86	9.8	10.4	10.2	10.2
Stdev	0.74	0.551	9.88	0.913	1.16
Number	111	75	12	11	9
z > 3	5	0	3	1	1
z 2 - 3	4	2	2	0	0

Sample 4					
Method	All*	IC	TITR	COLOR	CLR-A
Median	27.9	27.8	28.4	28.8	26.9
Stdev	2.09	1.21	3.13	2.12	1.24
Number	112	75	12	11	10
z > 3	2	0	1	1	0
z 2 - 3	2	1	1	0	0


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

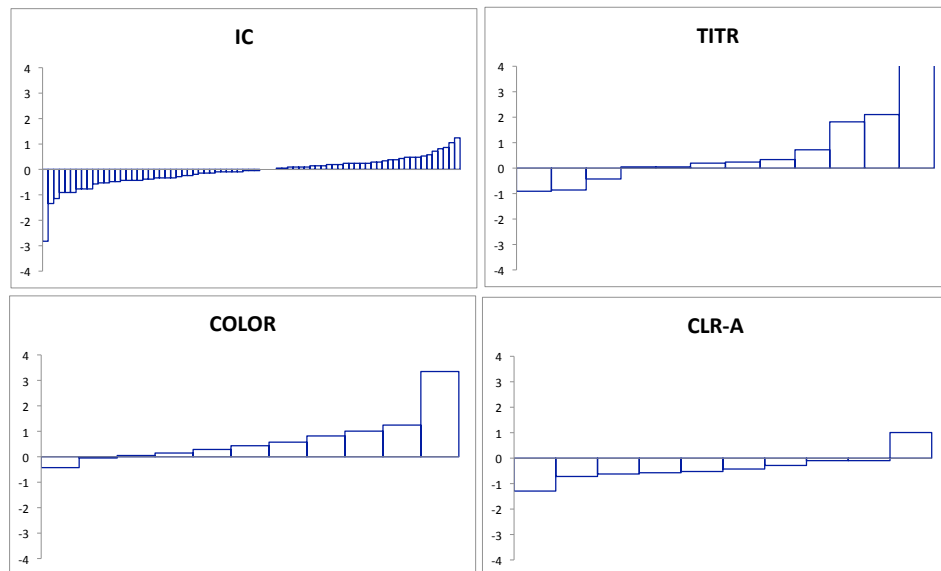


Conductivity (25 °C)

Kernel Density Plots

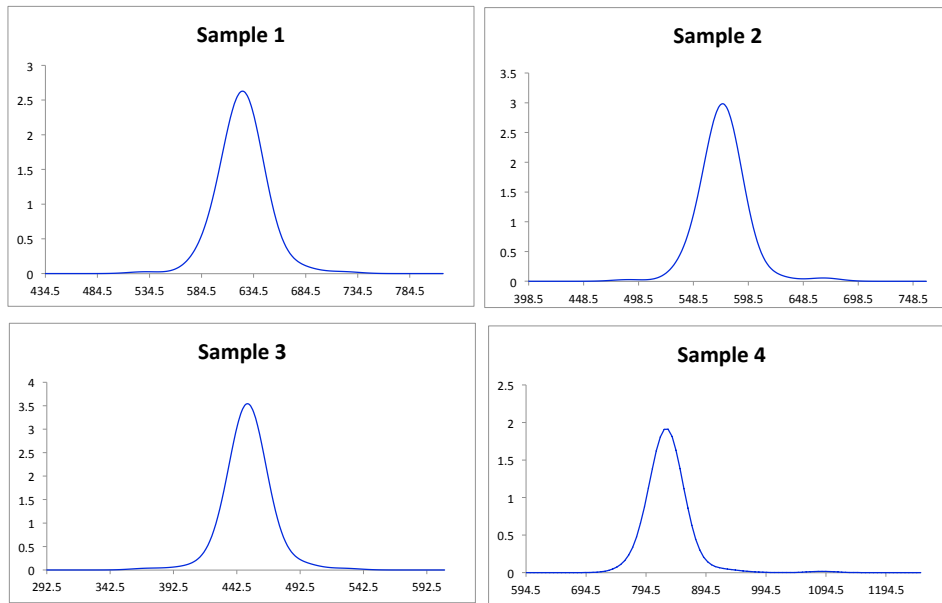

z-Score Plots

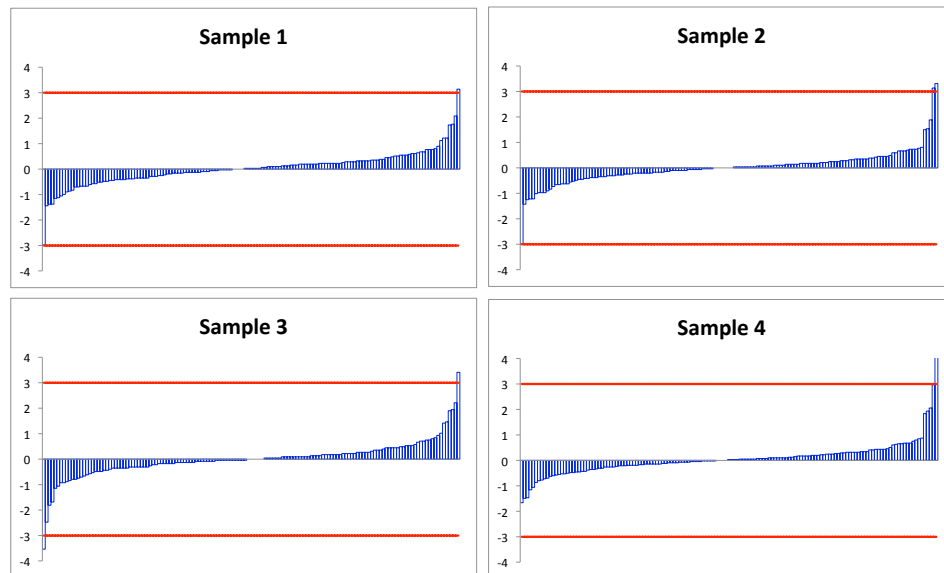

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	C-MTR	CA-MTR		
Median	623	625	619	0	0
Stdev	31.2	20.7	20.6	0	0
Number	145	126	19	0	0
z > 3	1	1	0	0	0
z 2 - 3	2	2	0	0	0


Sample 2					
Method	All*	C-MTR	CA-MTR		
Median	575	576	569	0	0
Stdev	28.7	19.4	18	0	0
Number	145	126	19	0	0
z > 3	2	2	0	0	0
z 2 - 3	1	1	0	0	0

Sample 3					
Method	All*	C-MTR	CA-MTR		
Median	451	452	448	0	0
Stdev	22.6	16.5	15.7	0	0
Number	145	126	19	0	0
z > 3	2	2	0	0	0
z 2 - 3	2	2	0	0	0

Sample 4					
Method	All*	C-MTR	CA-MTR		
Median	828	830	823	0	0
Stdev	41.4	33	24.8	0	0
Number	145	126	19	0	0
z > 3	1	1	0	0	0
z 2 - 3	2	1	1	0	0


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

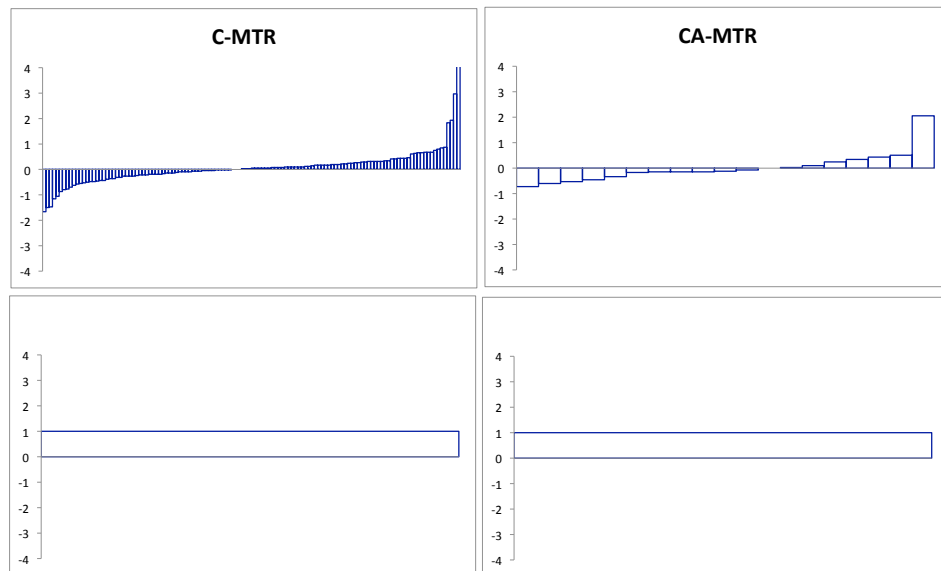


Fluoride

Kernel Density Plots

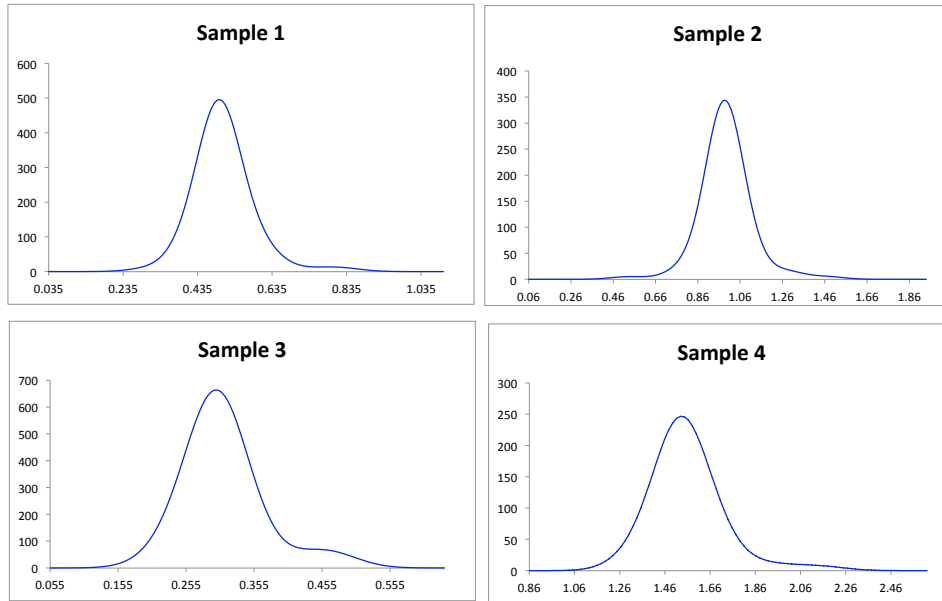

z-Score Plots

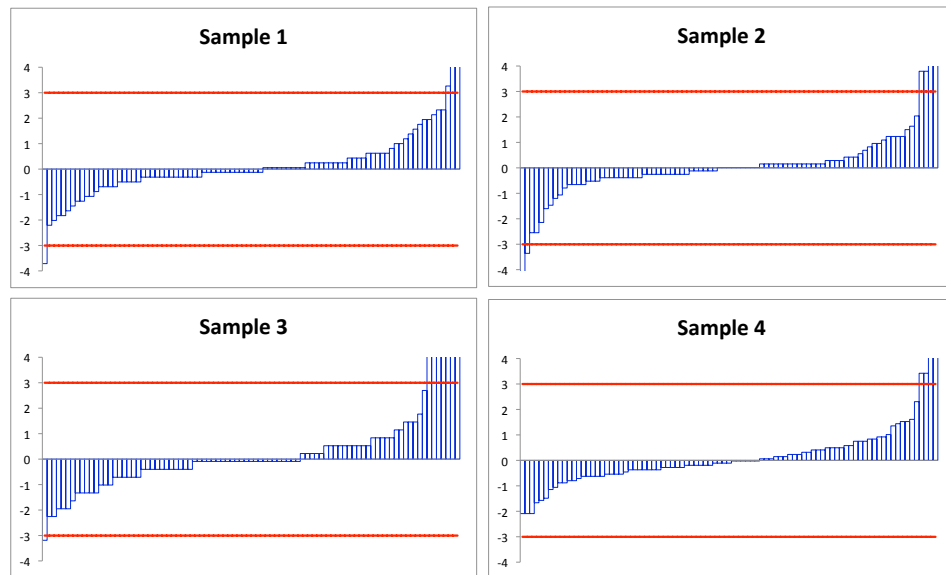

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	IC	SIE	COLOR	TITR
Median	0.497	0.49	0.5	0.6	0.49
Stdev	0.053	0.0618	0.0466	0.162	0
Number	89	53	30	5	1
z > 3	4	2	0	2	0
z 2 - 3	5	2	2	1	0


Sample 2					
Method	All*	IC	SIE	COLOR	TITR
Median	0.989	0.99	0.99	1	0.95
Stdev	0.0741	0.0903	0.104	0.271	0
Number	89	53	30	5	1
z > 3	6	1	3	2	0
z 2 - 3	4	4	0	0	0

Sample 3					
Method	All*	IC	SIE	COLOR	TITR
Median	0.303	0.3	0.31	0.46	0.3
Stdev	0.0323	0.0445	0.0262	0.0228	0
Number	89	53	30	5	1
z > 3	8	3	0	5	0
z 2 - 3	3	3	0	0	0

Sample 4					
Method	All*	IC	SIE	COLOR	TITR
Median	1.54	1.53	1.53	1.72	1.51
Stdev	0.116	0.125	0.136	0.204	0
Number	89	53	30	5	1
z > 3	4	1	2	1	0
z 2 - 3	4	2	1	1	0


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

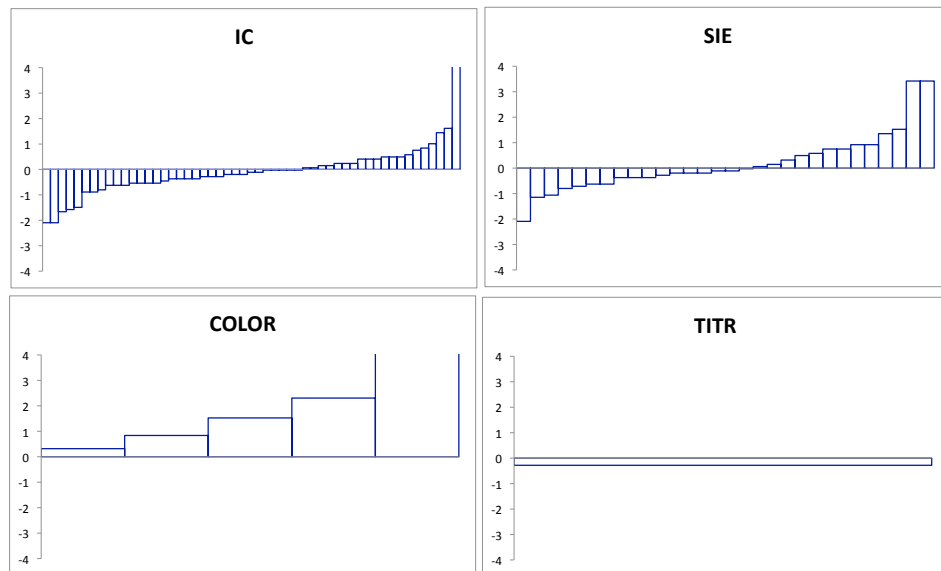


Hardness (as CaCO₃)

Kernel Density Plots

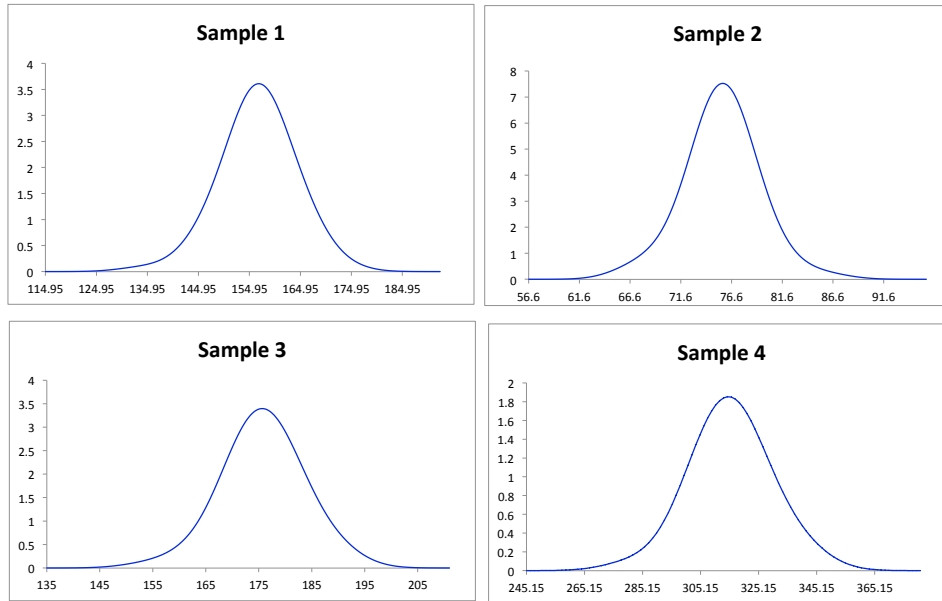

z-Score Plots

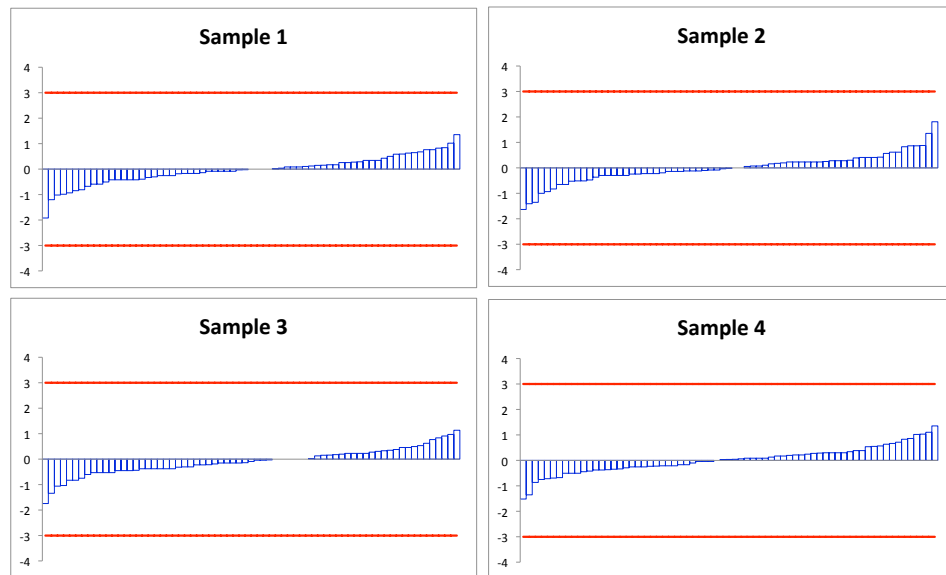

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	CALC	TITR	CALC(ICP)	TITR-A
Median	157	156	158	159	157
Stdev	11.8	6.79	5.75	10.5	0.707
Number	69	48	17	2	2
z > 3	0	0	0	0	0
z 2 - 3	0	0	0	0	0


Sample 2					
Method	All*	CALC	TITR	CALC(ICP)	TITR-A
Median	75.7	75.6	76.8	76.6	74
Stdev	5.68	3.38	3.25	3.68	0
Number	69	48	17	2	2
z > 3	0	0	0	0	0
z 2 - 3	0	0	0	0	0

Sample 3					
Method	All*	CALC	TITR	CALC(ICP)	TITR-A
Median	177	175	177	177	176
Stdev	13.2	7.39	5.83	8.84	1.41
Number	69	48	17	2	2
z > 3	0	0	0	0	0
z 2 - 3	0	0	0	0	0

Sample 4					
Method	All*	CALC	TITR	CALC(ICP)	TITR-A
Median	315	316	316	319	316
Stdev	23.6	13.4	11	16	2.12
Number	69	48	17	2	2
z > 3	0	0	0	0	0
z 2 - 3	0	0	0	0	0


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

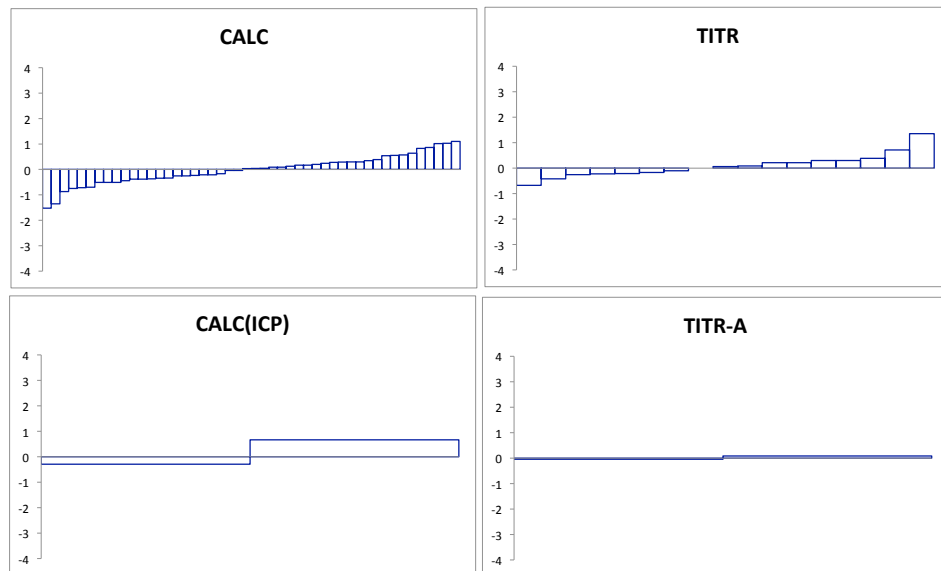


Inorganic Carbon

Kernel Density Plots

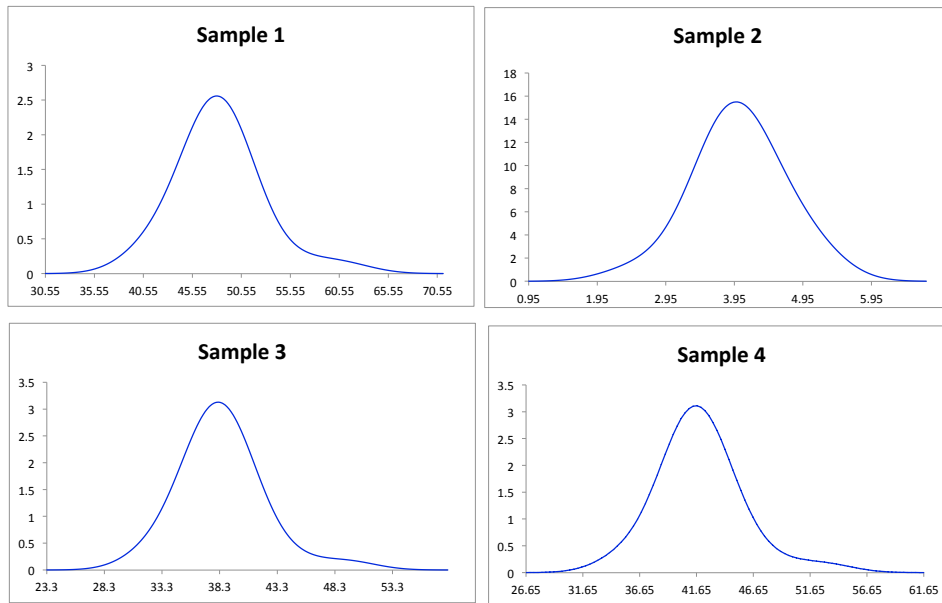

Z-Score Plots

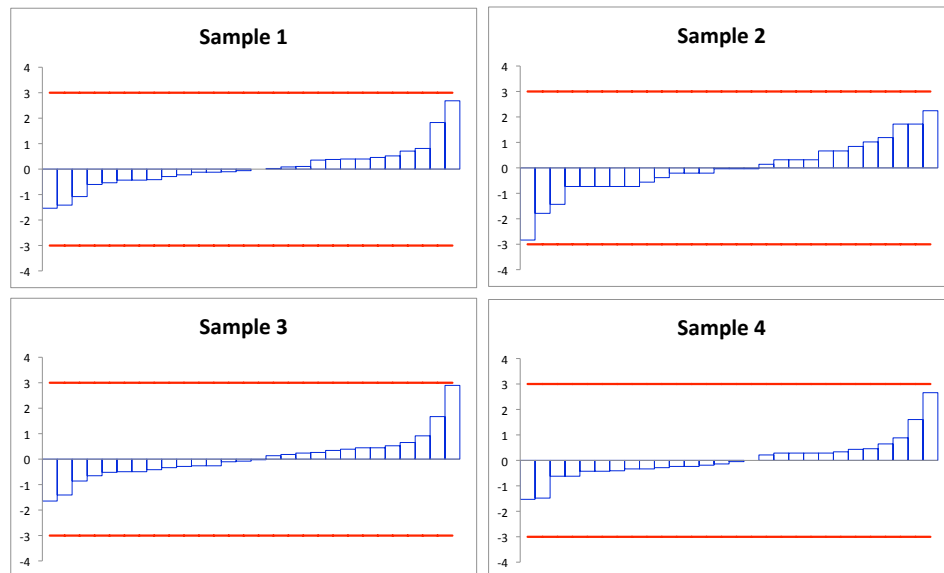

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	INFRARED	CALC	CLR-A	
Median	48.1	48	46.7	52	0
Stdev	4.81	4.19	0	0	0
Number	28	26	1	1	0
z > 3	0	0	0	0	0
z 2 - 3	1	1	0	0	0


Sample 2					
Method	All*	INFRARED	CALC	CLR-A	
Median	4.02	4	3.2	3	0
Stdev	0.571	0.586	0	0	0
Number	28	26	1	1	0
z > 3	0	0	0	0	0
z 2 - 3	2	2	0	0	0

Sample 3					
Method	All*	INFRARED	CALC	CLR-A	
Median	38.3	38.1	36.3	40	0
Stdev	3.83	3.44	0	0	0
Number	28	26	1	1	0
z > 3	0	0	0	0	0
z 2 - 3	1	1	0	0	0

Sample 4					
Method	All*	INFRARED	CALC	CLR-A	
Median	41.8	41.4	40.4	43	0
Stdev	4.18	3.53	0	0	0
Number	28	26	1	1	0
z > 3	0	0	0	0	0
z 2 - 3	1	1	0	0	0


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

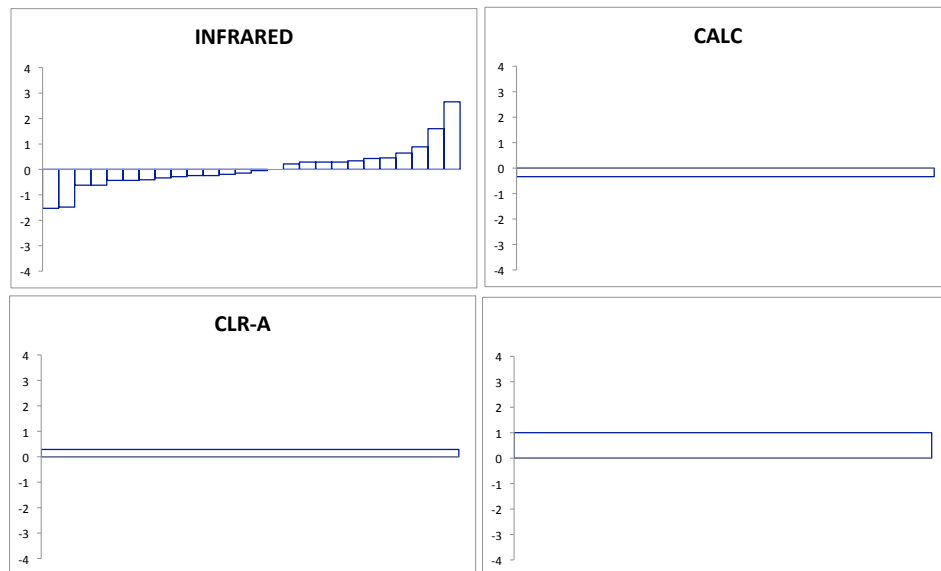


Magnesium

Kernel Density Plots

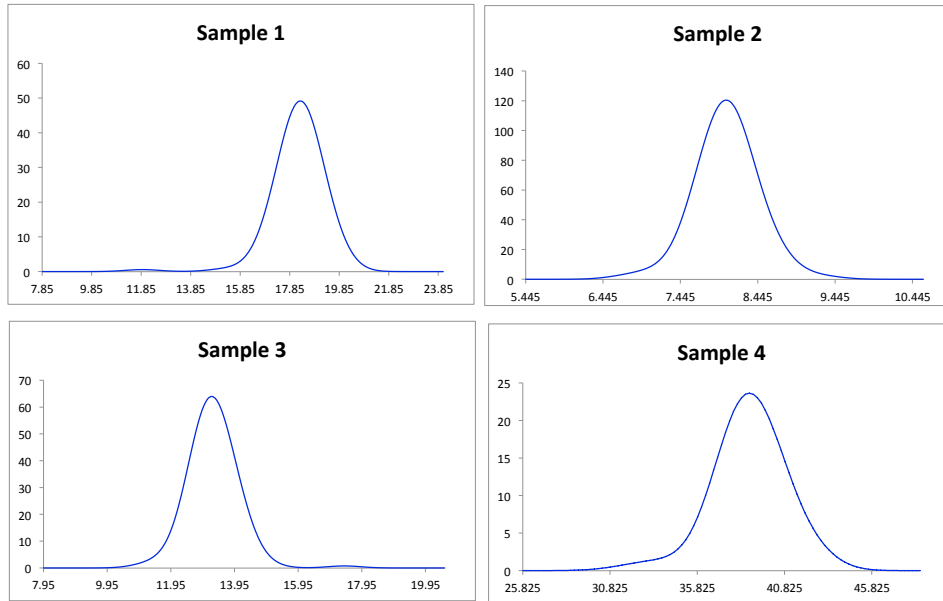

z-Score Plots

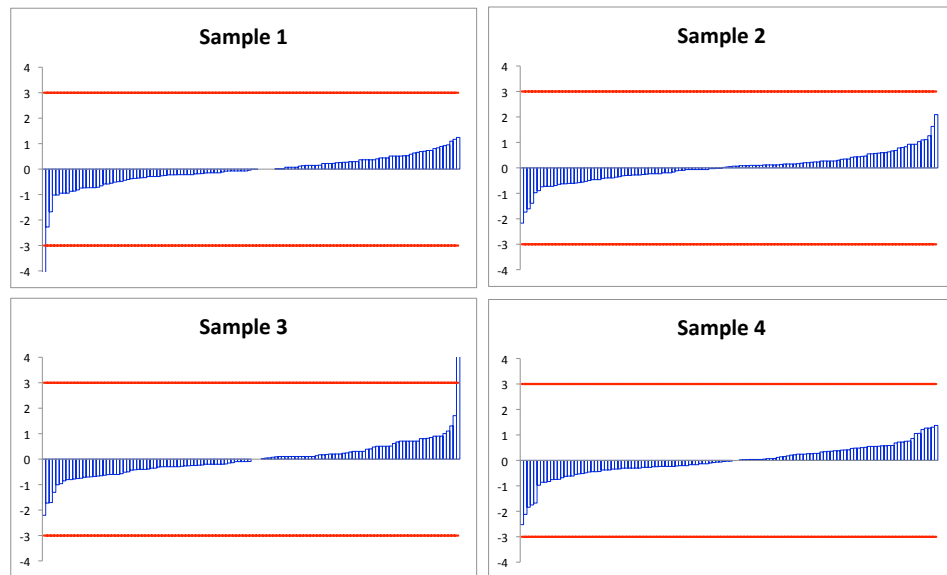

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	18.3	18.3	18.2	17.8	18
Stdev	1.37	0.824	0.717	0.505	3.17
Number	124	66	47	6	4
z > 3	1	0	0	0	1
z 2 - 3	1	1	0	0	0


Sample 2					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	8.04	8.07	8.1	7.69	7.91
Stdev	0.603	0.343	0.369	0.313	0.622
Number	124	66	47	6	4
z > 3	0	0	0	0	0
z 2 - 3	2	1	1	0	0

Sample 3					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	13.3	13.3	13.4	12.7	12.8
Stdev	0.995	0.784	0.622	0.381	0.204
Number	124	66	47	6	4
z > 3	1	1	0	0	0
z 2 - 3	1	1	0	0	0

Sample 4					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	38.9	39.1	38.4	38.5	37.8
Stdev	2.92	1.84	1.76	0.99	3.47
Number	124	66	47	6	4
z > 3	0	0	0	0	0
z 2 - 3	2	1	0	0	1


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

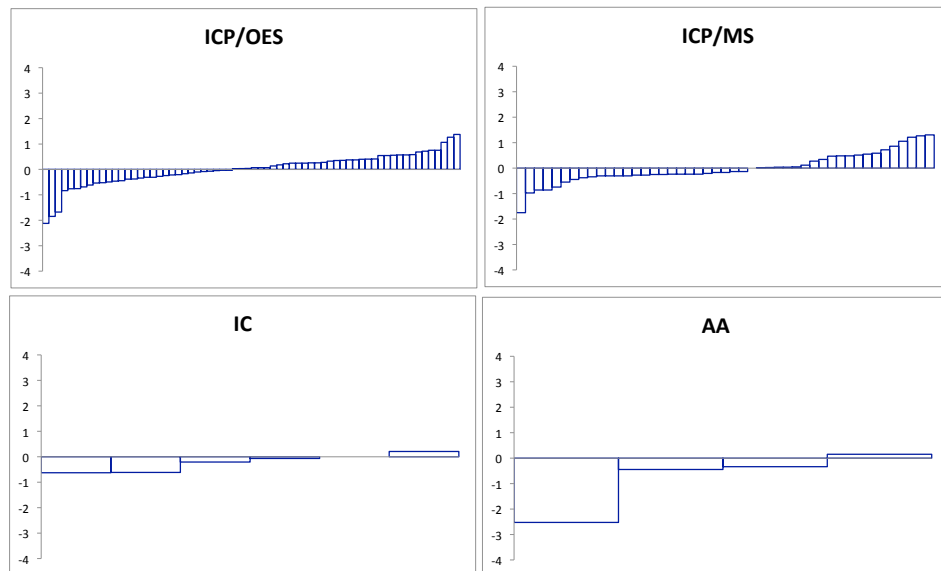


Nitrate

Kernel Density Plots

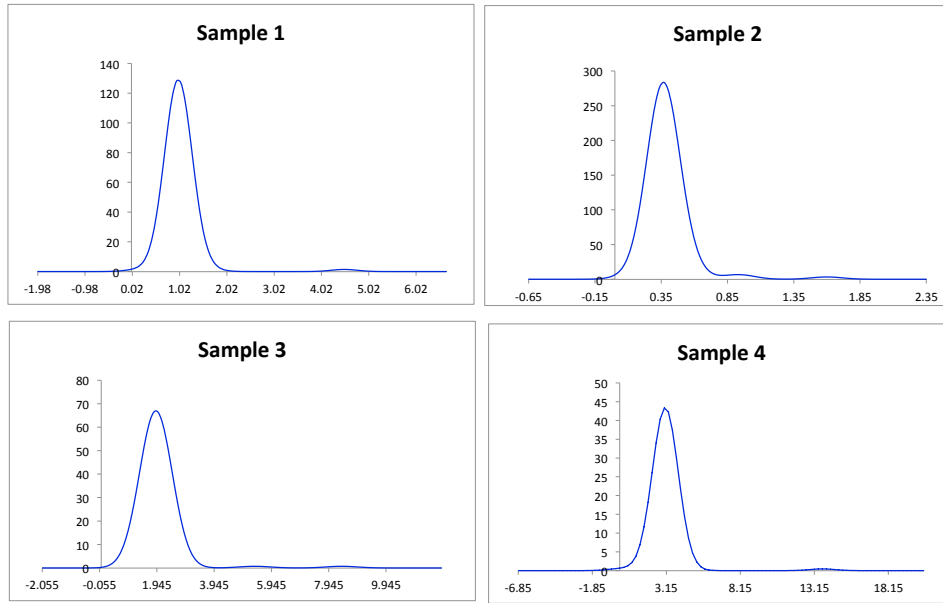

z-Score Plots

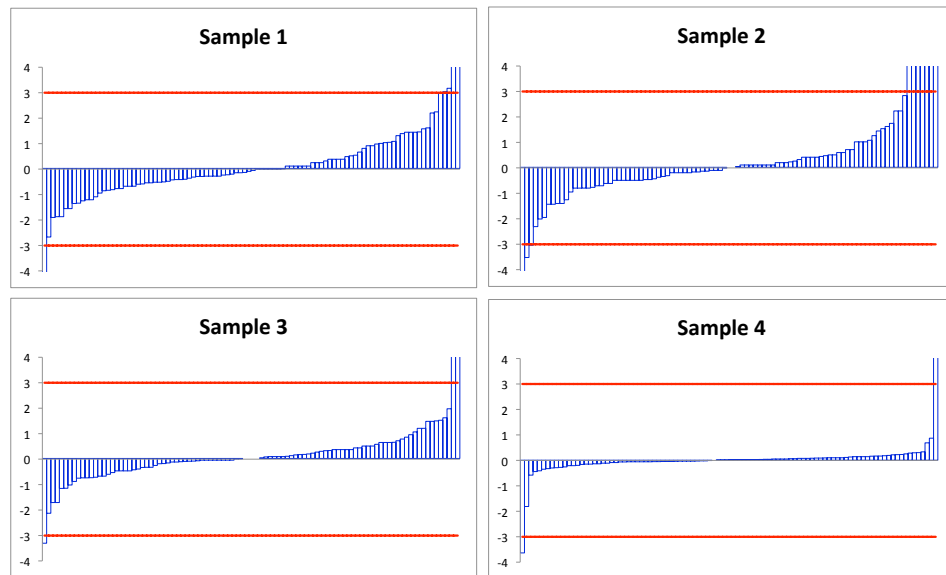

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	IC	COLOR	CLR-A	
Median	0.993	0.983	1.07	0.958	0
Stdev	0.0753	0.0735	0.803	0.0641	0
Number	98	66	19	12	0
z > 3	5	1	3	0	0
z 2 - 3	4	3	1	0	0


Sample 2					
Method	All*	IC	COLOR	CLR-A	
Median	0.367	0.363	0.37	0.367	0
Stdev	0.033	0.0529	0.326	0.0286	0
Number	95	65	18	11	0
z > 3	10	5	4	0	0
z 2 - 3	5	4	1	0	0

Sample 3					
Method	All*	IC	COLOR	CLR-A	
Median	1.91	1.91	1.9	1.9	0
Stdev	0.144	0.0869	1.5	0.0926	0
Number	98	66	19	12	0
z > 3	3	0	2	0	0
z 2 - 3	1	1	0	0	0

Sample 4					
Method	All*	IC	COLOR	CLR-A	
Median	3.08	3.09	3.06	3.13	0
Stdev	0.846	0.122	2.48	0.126	0
Number	98	66	19	12	0
z > 3	2	0	1	0	0
z 2 - 3	0	0	0	0	0

* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.


z-Score Plots by Method - Sample 4

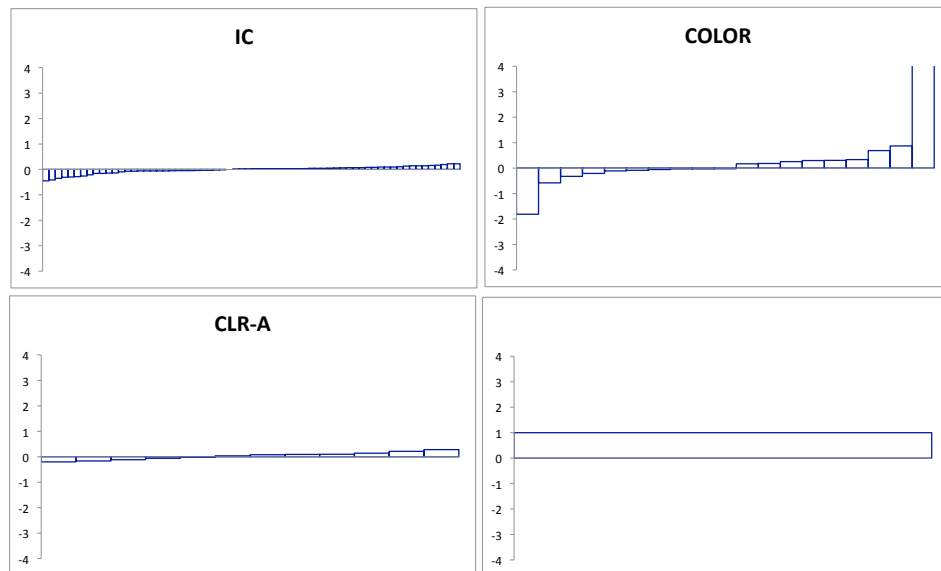


Evaluation for sample 4 was adjusted for stability flag.

Nitrate plus Nitrite

Kernel Density Plots

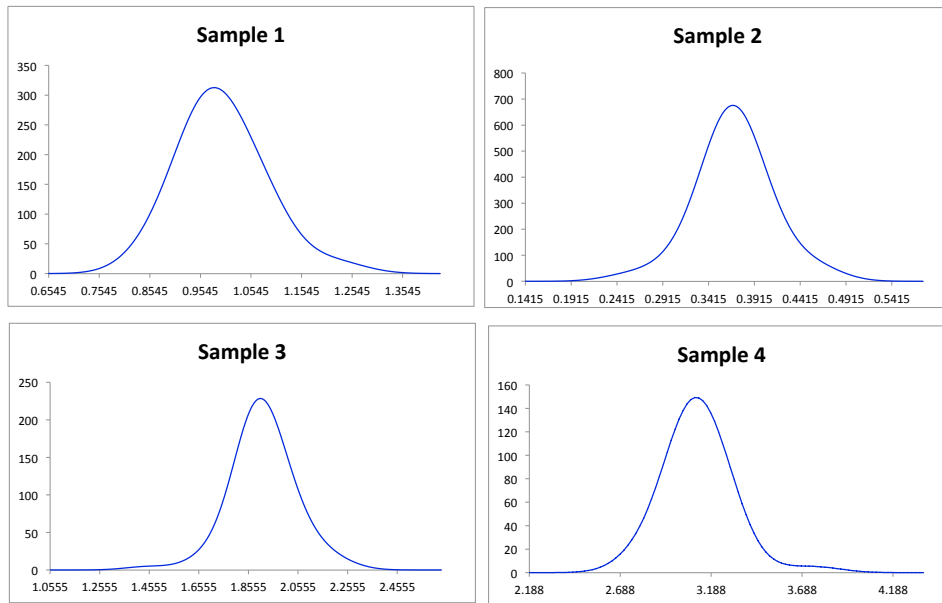

z-Score Plots

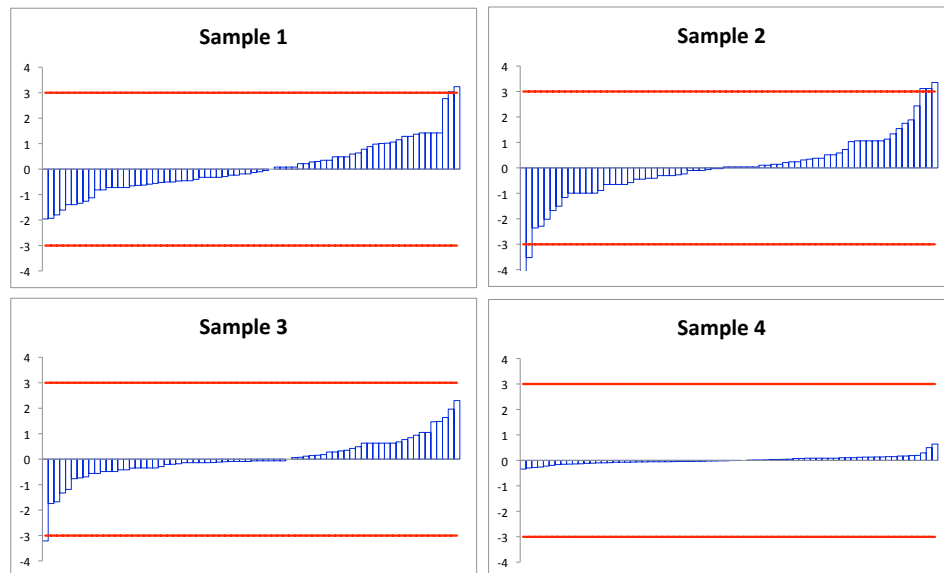

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	IC	CLR-A	COLOR	CALC
Median	0.994	0.964	1	0.976	0.997
Stdev	0.0745	0.0773	0.0628	0.0972	0.0184
Number	72	25	23	22	2
z > 3	2	1	0	1	0
z 2 - 3	1	0	0	1	0


Sample 2					
Method	All*	IC	CLR-A	COLOR	CALC
Median	0.369	0.362	0.37	0.37	0.42
Stdev	0.0292	0.0474	0.0243	0.0335	0.0566
Number	70	25	22	21	2
z > 3	5	3	0	1	1
z 2 - 3	4	2	0	2	0

Sample 3					
Method	All*	IC	CLR-A	COLOR	CALC
Median	1.91	1.9	1.9	1.9	1.94
Stdev	0.143	0.0906	0.075	0.176	0.0127
Number	72	25	23	22	2
z > 3	1	0	0	1	0
z 2 - 3	1	0	0	1	0

Sample 4					
Method	All*	IC	CLR-A	COLOR	CALC
Median	3.11	3.09	3.14	3.07	3.11
Stdev	1.1	0.142	0.129	0.237	0.0707
Number	72	25	23	22	2
z > 3	0	0	0	0	0
z 2 - 3	0	0	0	0	0

* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.


z-Score Plots by Method - Sample 4

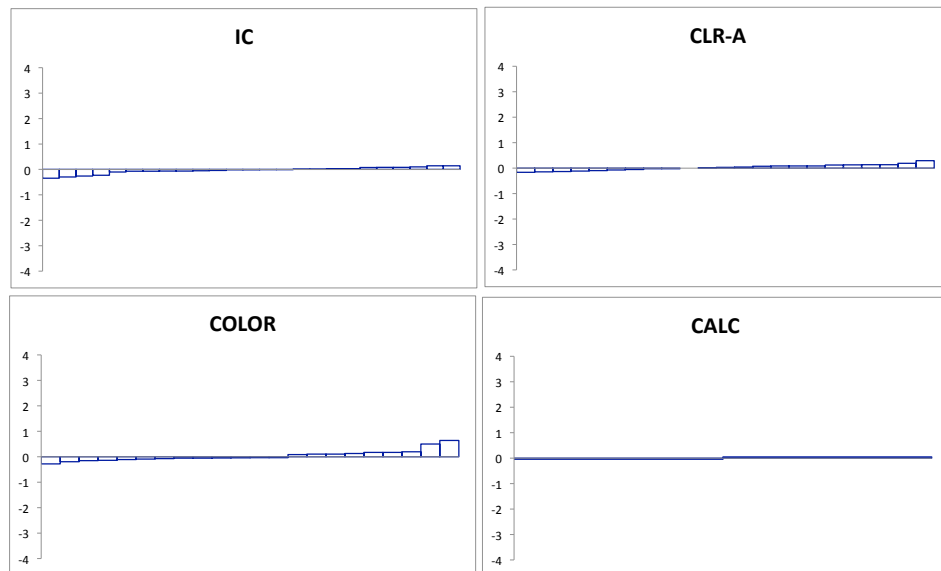


Evaluations for sample 4 was adjusted for stability flags.

Potassium

Kernel Density Plots

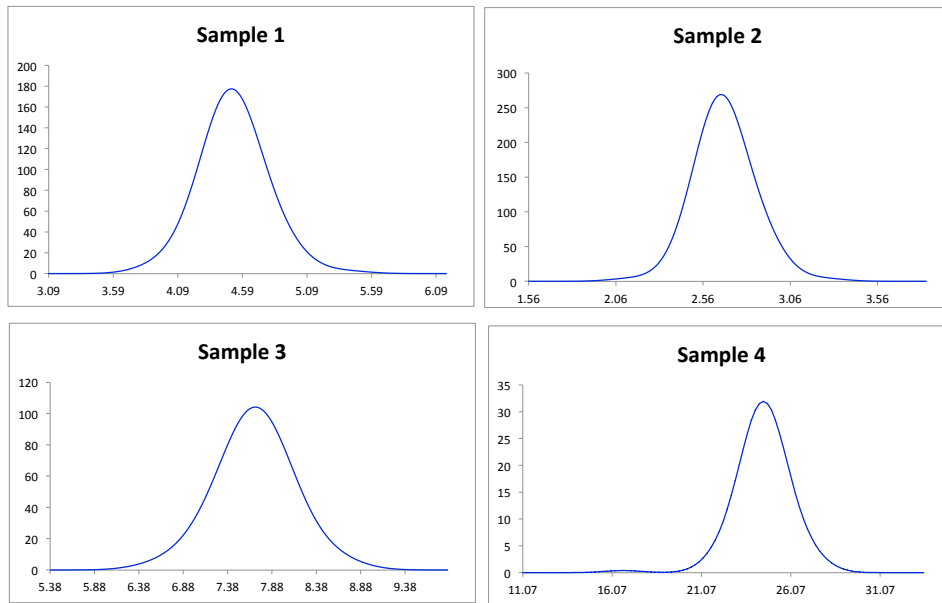

z-Score Plots

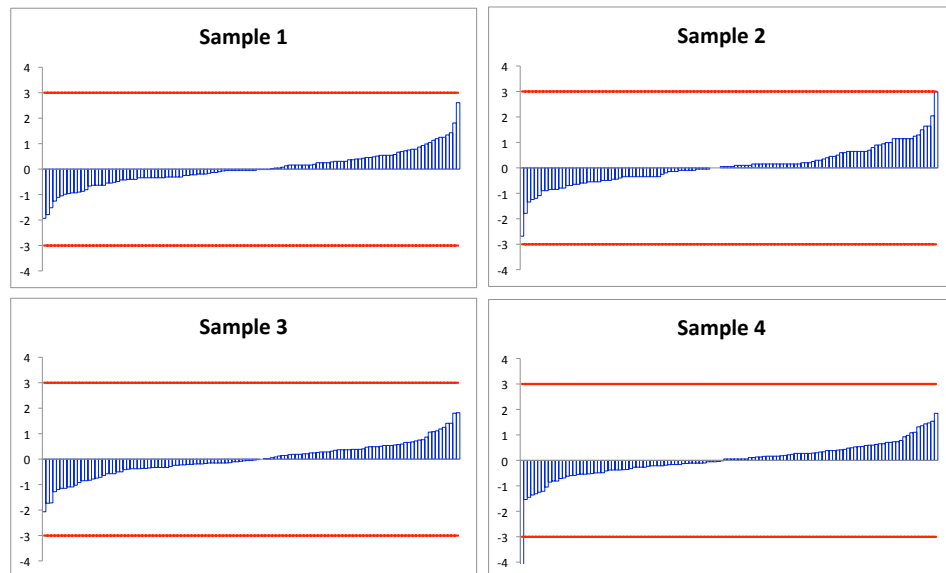

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	4.52	4.48	4.52	4.45	4.56
Stdev	0.339	0.233	0.241	0.118	0.176
Number	119	61	46	6	4
z > 3	0	0	0	0	0
z 2 - 3	1	0	1	0	0


Sample 2					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	2.67	2.68	2.69	2.58	2.76
Stdev	0.201	0.173	0.137	0.0458	0.106
Number	119	61	46	6	4
z > 3	0	0	0	0	0
z 2 - 3	3	2	1	0	0

Sample 3					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	7.69	7.65	7.79	7.53	7.57
Stdev	0.576	0.35	0.461	0.162	0.252
Number	119	61	46	6	4
z > 3	0	0	0	0	0
z 2 - 3	1	0	1	0	0

Sample 4					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	24.5	24.3	24.7	24.5	24.3
Stdev	1.84	1.02	1.33	0.366	4.27
Number	119	61	46	6	4
z > 3	1	0	0	0	1
z 2 - 3	0	0	0	0	0


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

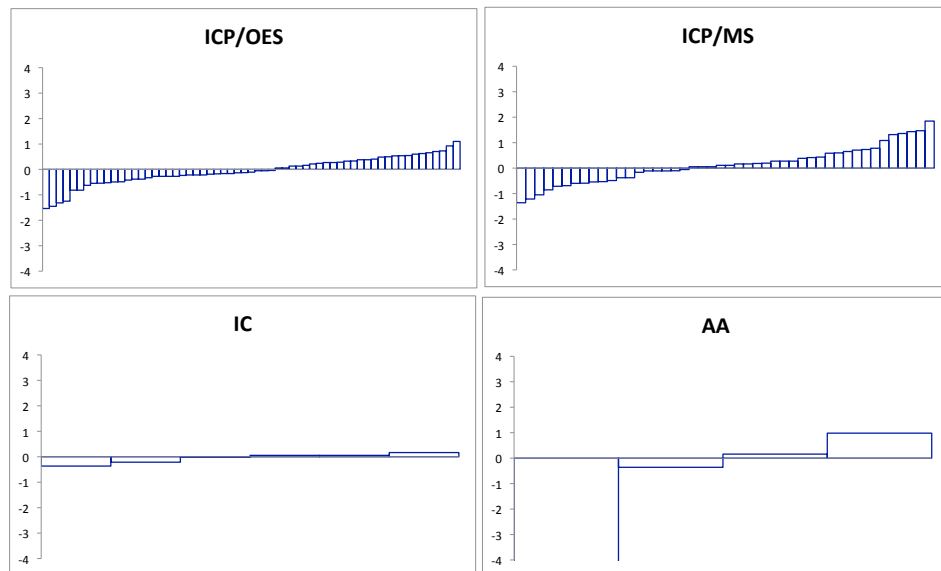


Reactive Silica

Kernel Density Plots

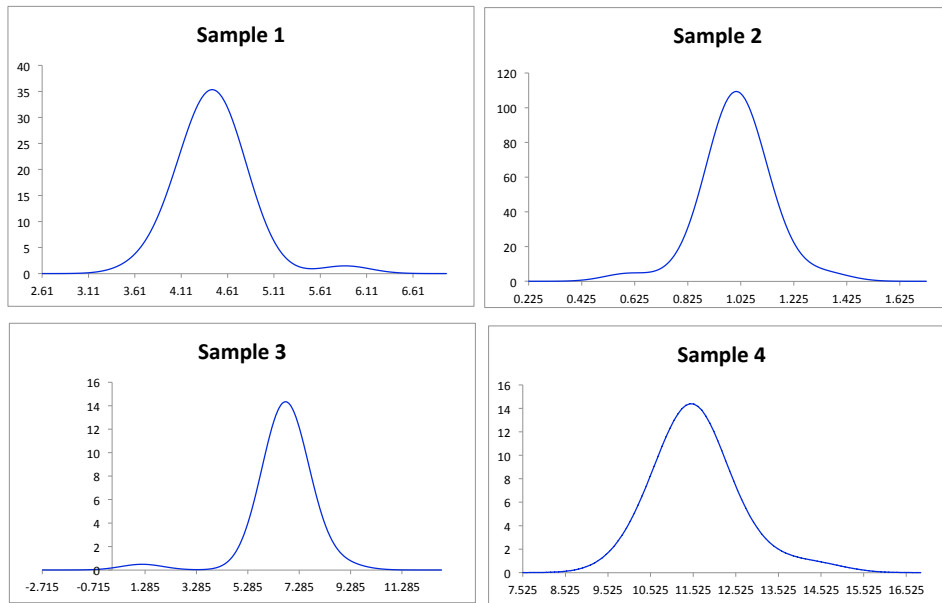

z-Score Plots

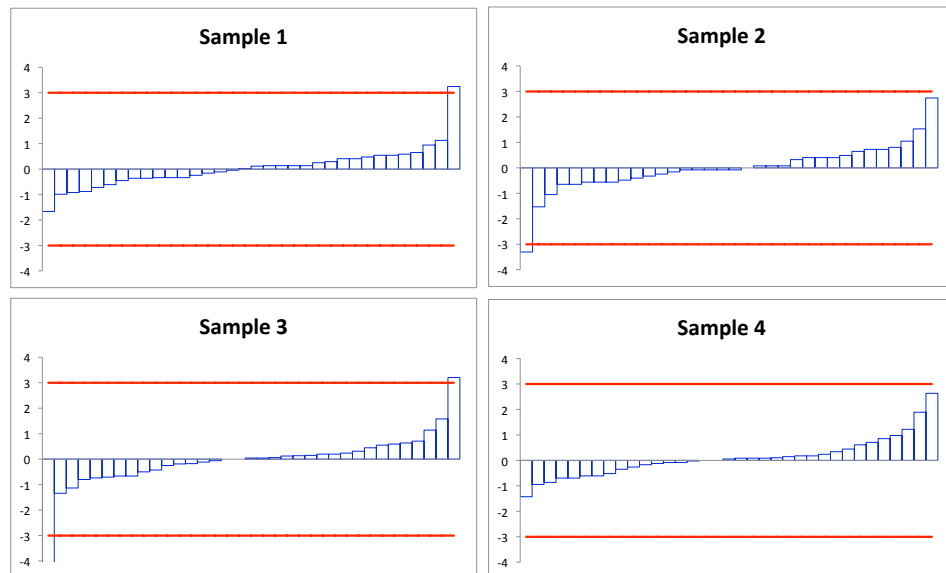

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	CLR-A	COLOR	CALC	
Median	4.44	4.53	4.46	4.31	0
Stdev	0.444	0.475	0.245	0.201	0
Number	34	16	10	8	0
z > 3	1	1	0	0	0
z 2 - 3	0	0	0	0	0


Sample 2					
Method	All*	CLR-A	COLOR	CALC	
Median	1.01	1	1.04	0.995	0
Stdev	0.124	0.165	0.062	0.061	0
Number	34	16	10	8	0
z > 3	1	1	0	0	0
z 2 - 3	1	1	0	0	0

Sample 3					
Method	All*	CLR-A	COLOR	CALC	
Median	6.77	6.9	6.77	6.61	0
Stdev	0.677	0.687	1.73	0.332	0
Number	35	16	11	8	0
z > 3	2	1	1	0	0
z 2 - 3	0	0	0	0	0

Sample 4					
Method	All*	CLR-A	COLOR	CALC	
Median	11.5	11.6	11.6	11.1	0
Stdev	1.15	0.942	0.999	0.566	0
Number	35	16	11	8	0
z > 3	0	0	0	0	0
z 2 - 3	1	0	1	0	0

* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.


z-Score Plots by Method - Sample 4

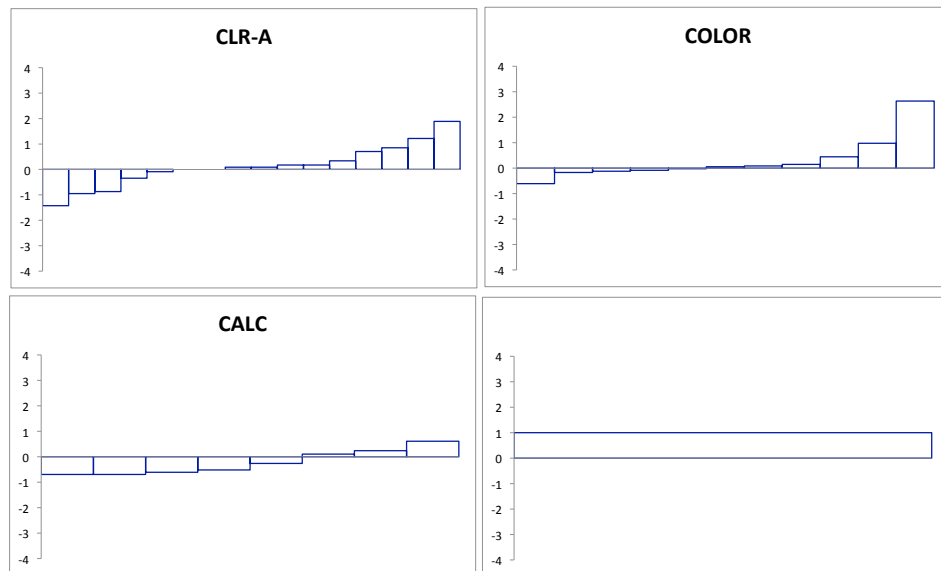


Evaluation for sample 2 was adjusted for stability flags.

Sodium

Kernel Density Plots

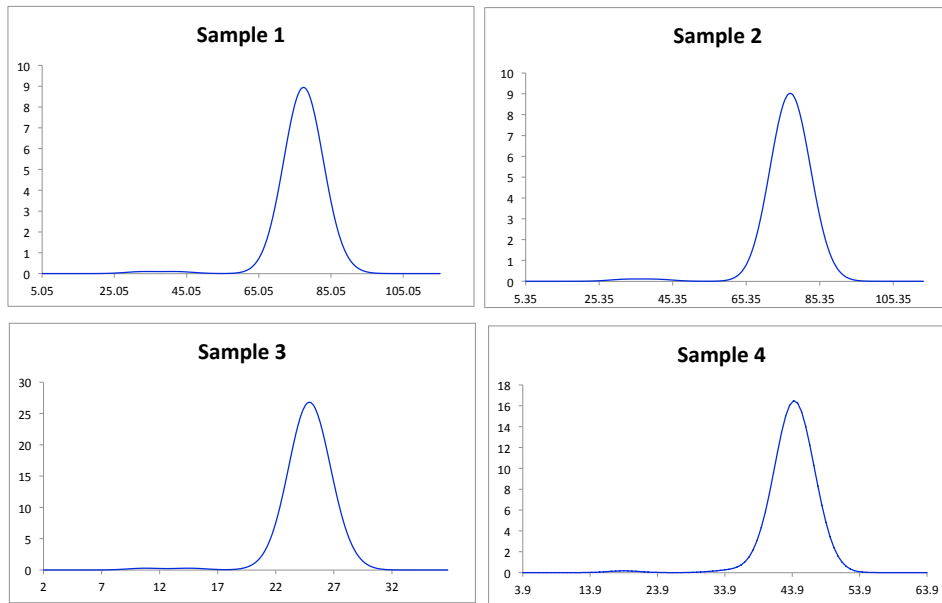

z-Score Plots

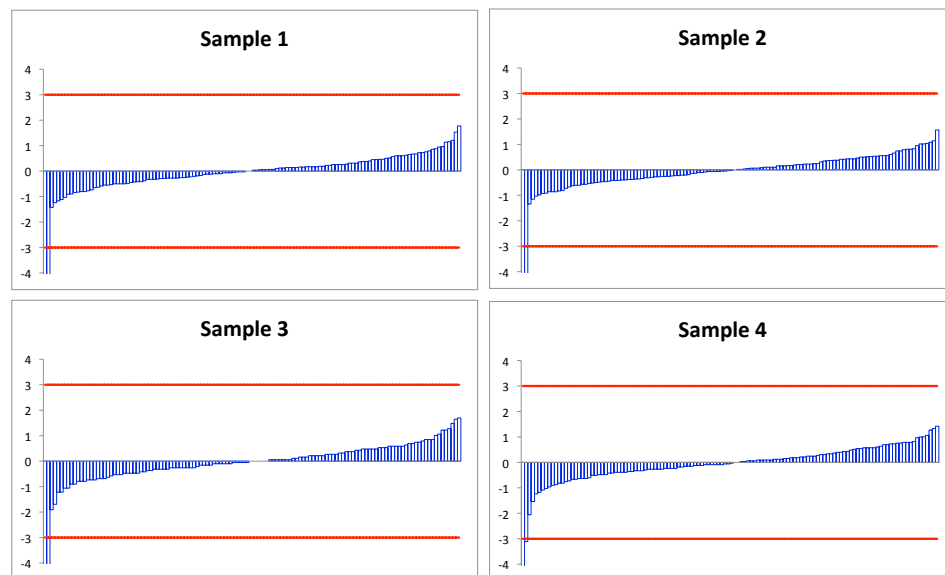

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	77.4	77	77.7	77.1	77.5
Stdev	5.81	6.57	3.24	1.16	18.4
Number	126	65	46	7	4
z > 3	2	1	0	0	1
z 2 - 3	0	0	0	0	0


Sample 2					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	77.4	77	77.8	76.3	76.4
Stdev	5.8	6.43	3.06	1.12	19.1
Number	126	65	46	7	4
z > 3	2	1	0	0	1
z 2 - 3	0	0	0	0	0

Sample 3					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	24.9	24.9	25	24.6	23.2
Stdev	1.89	2.08	1.27	0.435	5.3
Number	126	65	46	7	4
z > 3	2	1	0	0	1
z 2 - 3	0	0	0	0	0

Sample 4					
Method	All*	ICP/OES	ICP/MS	IC	AA
Median	44.2	44.4	44.2	43.7	40.3
Stdev	3.31	3.68	1.97	0.63	5.08
Number	126	65	46	7	4
z > 3	2	1	0	0	1
z 2 - 3	1	0	0	0	1


* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

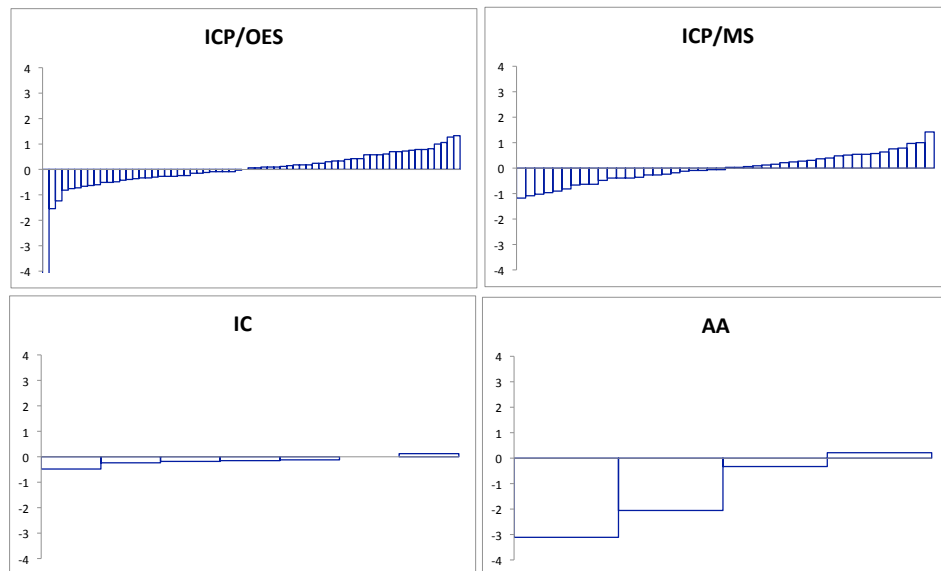


Sulfate

Kernel Density Plots

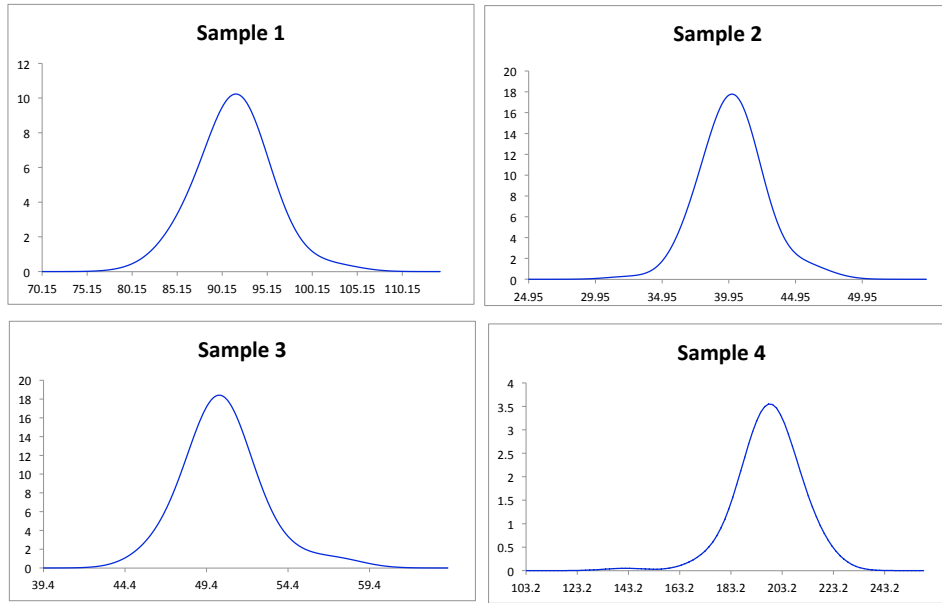

z-Score Plots

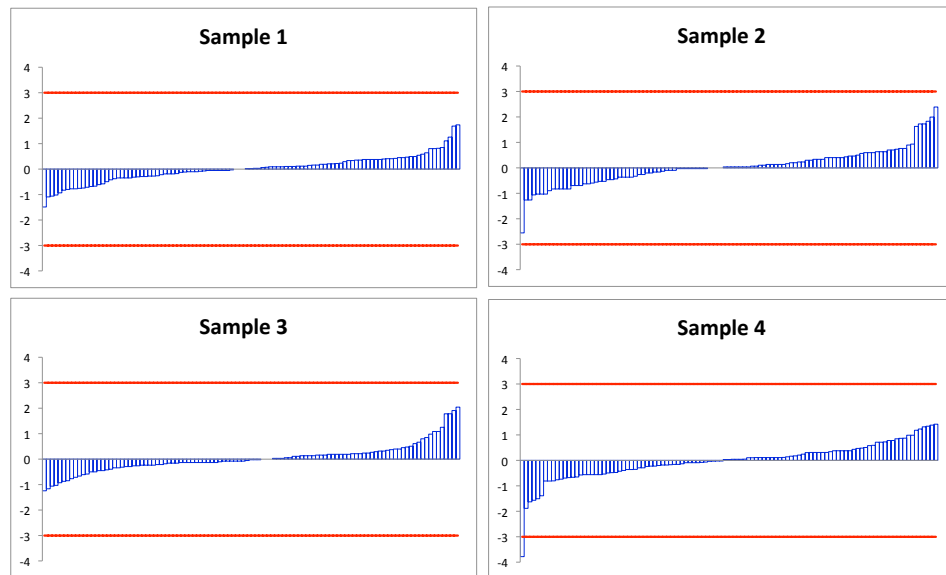

Summary Statistics by Four Most Common Methods

Sample 1					
Method	All*	IC	COLOR	CALC	TURB
Median	91.4	91.5	91.6	88	93.2
Stdev	6.86	3.02	5.82	3.31	6.2
Number	107	78	9	8	8
z > 3	0	0	0	0	0
z 2 - 3	0	0	0	0	0

Sample 2					
Method	All*	IC	COLOR	CALC	TURB
Median	40.1	40.2	39	39	41.2
Stdev	3.01	1.94	3.04	1.48	3.1
Number	107	78	9	8	8
z > 3	0	0	0	0	0
z 2 - 3	2	2	0	0	0

Sample 3					
Method	All*	IC	COLOR	CALC	TURB
Median	50.3	50	54.4	48.9	51.1
Stdev	3.77	1.5	3.19	1.56	2.9
Number	107	78	9	8	8
z > 3	0	0	0	0	0
z 2 - 3	1	0	0	0	1

Sample 4					
Method	All*	IC	COLOR	CALC	TURB
Median	198	199	203	188	203
Stdev	14.9	8.12	24	10.2	10.9
Number	107	78	9	8	8
z > 3	1	0	1	0	0
z 2 - 3	0	0	0	0	0

* Values for the median and standard deviation are the robust mean and acceptance limit deviation. For method statistics, the arithmetic mean and standard deviation are used.

z-Score Plots by Method - Sample 4

